

Product Portfolio Boditech Med Inc.

Advanced Compact Immunofluorescence Analyzer

ichroma™ II

- ▶ High performance with reliability
- ▶ Small, compact & light
- ▶ Multi-test function
- ▶ LIS/HIS compatible



Specifications

QC/Calibration

- System check cartridge
- Internal & external controls

Interface

- 7" touch screen
- Built-in thermal printer
- USB port / USB OTG port / Ethernet
- SD card slot / WiFi
- LIS / HIS compatible

Memory

- 1,000 patient results
- 1,000 QC results
- 100 User IDs

Analyzer

- 276 x 220 x 91 mm
- 1.3 kg
- 100 – 240 V AC, 50-60 Hz
- Battery (AAx4)

High-throughput Immunofluorescence Analyzer

ichroma™ III

- ▶ Random access for various parameters
- ▶ Continuous testing
- ▶ Flexible temperature control
- ▶ Patient ID handwriting for user convenience
- ▶ ID chip memory function

Specifications

QC/Calibration

- System check cartridge
- Internal & external controls

Interface

- 7" touch screen
- Built-in thermal printer
- USB port / Ethernet
- SD card slot / RS232C port
- LIS/HIS compatible

Memory

- 5,000 patients results
- 500 ID chips
- 100 User IDs

Analyzer

- 240 x 465 x 341 mm
- 11 kg
- 100-240 V AC, 50-60 Hz
- Internal temperature control



World First Automated Dry Immunoassay System

ichroma™ -50 PLUS

- ▶ Full automation from sample to result
- ▶ High throughput
 - Capable of processing up to 20 individuals per hour for IGRA-TB test
- ▶ Ready for universal blood collection tube
- ▶ Various types of sample
 - Whole blood, fingertip blood, serum, plasma and stool



Specifications

QC/Calibration

- Internal & external controls

Interface

- 10.1-inch TFT LCD (touch screen)
- Built-in thermal printer
- USB port / Ethernet
- SD card slot / RS232 port
- LIS/HIS compatible

Memory

- 10,000 test results

Analyzer

- 622.5 x 612.6 x 470 mm
- 55 kg
- 100-240 V AC, 50/60 Hz

Handheld Fluorescence Immuno-analyzer

Portable and compact with high performance
One-click operation for user convenience

ichroma™ M2 ichroma™ M3

- ▶ Specialized in respiratory and infectious testing
- ▶ Ideal for mobile and field diagnostics
- ▶ Built-in heating system ensures stable test conditions
- ▶ Optimized for non-communicable disease management in primary care settings

Specifications

QC/Calibration

- System check cartridge
- Internal & external controls

Interface

- One-button operation
- LCD display

Analyzer

- 165 x 95 x 55 mm
- 300 g (M2) & 312 g (M3)
- 100-240 V AC, 50-60 Hz



ichroma™ Parameters

Category	Item	ichroma™ II	ichroma™ III	ichroma™ M2	ichroma™ M3	Sample type	Capillary Tube	Working range	Test time (min)
Cardiac	LDL Cholesterol Direct	●	●			S/P		10-300 mg/dL	10
	hsCRP	●	●			WB/S/P		0.1-10 mg/L	3
	D-Dimer	●	●			WB/P		50-10,000 ng/mL	12
	D-Dimer Neo	●	●			WB/P		50-10,000 ng/mL	12
	Tn-I	●	●			S/P		0.1-50 ng/mL	12
	Tn-I Neo	●	●			S/P		0.1-50 ng/mL	12
	Tn-I Plus	●	●	●		WB/S/P	●	0.01-15 ng/mL	12
	CK-MB	●	●			WB/S/P		3-100 ng/mL	12
	CK-MB Neo	●	●			WB/S/P		3-100 ng/mL	12
	Myoglobin	●	●			WB/S/P		5-500 ng/mL	12
	Myoglobin Neo	●	●			WB/S/P		5-500 ng/mL	12
	Cardiac Triple	●	●			WB/S/P		Tn-I: 0.01-15 ng/mL CK-MB: 3-100 ng/mL Myoglobin: 5-500 ng/mL	12
	Troponin T	●	●	●		WB/S/P	●	10-20,000 pg/mL	12
	BNP	●	●	●		WB/P	●	5-5,000 pg/mL	12
	NT-proBNP	●	●	●		WB/S/P		10-30,000 pg/mL	12
	ST2	●	●			WB/S/P		3.1-200 ng/mL	12
Cancer	PSA	●				WB/S/P	●	S/P: 0.1-100 ng/mL (WB: 0.5-100 ng/mL)	15
	PSA Neo	●	●		●	WB/S/P	●	0.1-100 ng/mL	15
	Free PSA	●	●	●		WB/S/P	●	0.05-50 ng/mL	12
	AFP	●	●			WB/S/P		5-350 ng/mL	15
	AFP Neo	●	●			WB/S/P		5-350 ng/mL	15
	CEA	●	●			WB/S/P		1-500 ng/mL	15
	CEA Neo	●	●			WB/S/P		1-500 ng/mL	15
	iFOB Neo	●	●			Feces		25-1,000 ng/mL	10
	Cyfra21-1	●	●	●		S/P		1-500 ng/mL	12
	CA19-9	●	●	●		S/P		8-1,000 U/mL	12
	CA125	●	●	●		S/P		5-700 U/mL	12
Diabetes	HbA1c	●	●			WB	●	(NGSP) 4-15 %	12
	HbA1c Neo	●	●		●	WB	●	(NGSP) 4-15 %	12
	Microalbumin	●	●			Urine		2-300 mg/L	12
	Cystatin C	●	●			S/P		0.1-7.5 mg/L	10
	Insulin	●	●	●		WB/S/P	●	2-300 µIU/mL	12
Hormone	TSH	●	●		●	WB/S/P		0.09-100 µIU/mL	12
	TSH Plus	●	●	●		WB/S/P		0.1-50 µIU/mL	12
	T3	●	●		●	S/P		0.5-5 ng/mL (0.77-7.7 nmol/L)	8
	T4	●	●		●	S/P		10.23-300 nmol/L	8
	Free T4	●	●			WB/S/P		1-100 pmol/L	12
	FSH	●	●			S/P		1-100 mIU/mL	15
	Progesterone	●	●			S/P		4.45-127.2 nmol/L	15
	β-HCG	●	●			WB/S/P		5-50,000 mIU/mL	15
	β-HCG Plus	●	●	●		WB/S/P		2-5,000 mIU/mL	12
	LH	●	●			S/P		1.0-100 mIU/mL	15
	PRL	●	●			S/P		1-100 ng/mL	10
	Testosterone	●	●			S/P		0.5-12 ng/mL	12
	Cortisol	●	●			WB/S/P		50-800 nmol/L	10
	AMH	●	●	●		S/P		0.02-15 ng/mL	12
	Estradiol* New	●	●	●		WB/S/P		20-3,000 pg/mL	15
PTH	●	●	●		WB/S/P		30-3,000 pg/mL	12	

* No CE mark

WB = Whole blood, S = Serum, P = Plasma, NS = Nasopharyngeal swab

ichroma™ Parameters

Category	Item	ichroma™ II	ichroma™ III	ichroma™ M2	ichroma™ M3	Sample type	Capillary Tube	Working range	Test time (min)
Infection	CRP	●	●		●	WB/S/P		2.5-300 mg/L	3
	hsCRP All in one	●	●			WB/S/P		0.5-200 mg/L	3
	MxA/CRP	●	●			WB	●	MxA: 10-300 ng/mL CRP: 1-200 mg/L	12
	PCT	●	●			WB/S/P		0.1-100 ng/mL	12
	PCT Plus	●	●	●		WB/S/P	●	0.02-50 ng/mL	12
	PCT Plus G	●	●	●		WB/S/P	●	0.02-50 ng/mL	12
	IL-6	●	●	●		WB/S/P	●	2-2,500 pg/mL	12
	Influenza A+B	●	●	●		NS/ Nasal aspirate		Qualitative	10
	RSV	●	●	●		NS/ Nasal aspirate		Qualitative	10
	Influenza A+B/RSV	●	●	●		NS/ Nasal aspirate		Qualitative	10
	COVID-19 Ab	●	●	●		WB/S/P		Qualitative	10
	COVID-19 Ag	●	●	●		NS		Qualitative	12
	COVID-19/Flu Ag Combo	●	●	●		NS		Qualitative	20
	COVID-19/Flu A+B/ RSV Ag Combo	●	●	●		NS		Qualitative	20
	Adeno	●	●	●		NS/ Nasal aspirate		Qualitative	10
	Mycoplasma	●	●	●		Throat swab		Qualitative	10
	Strep A	●	●	●		Throat swab		Qualitative	5
	ASO	●	●			S/P		25-800 IU/mL	12
	HBsAg*	●				WB/S/P		Qualitative	12
	Anti-HBs*	●	●	●		WB/S/P		Qualitative	15
	Anti-HCV*	●				WB/S/P		Qualitative	12
	Dengue NS1Ag	●	●	●		WB/S/P		Qualitative	12
	Dengue IgG/IgM	●	●	●		WB/S/P		Qualitative	12
	Zika IgG/IgM	●	●	●		WB/S/P		Qualitative	12
	CHIKV IgG/IgM	●	●	●		WB/S/P		Qualitative	10
	Toxo IgM*	●	●	●		WB/S/P	●	Qualitative	12
	Toxo IgG*	●	●			WB/S/P	●	Qualitative	12
	Toxo IgG/IgM*	●	●			WB/S/P	●	Qualitative	12
	Rubella IgM*	●	●	●		WB/S/P	●	Qualitative	12
	Rubella IgG*	●	●	●		WB/S/P	●	Qualitative	12
	CMV IgM*	●	●	●		WB/S/P	●	Qualitative	12
	CMV IgG*	●	●	●		WB/S/P	●	Qualitative	12
IGRA-TB** (★)					P		Qualitative	15	
IGRA-TB 25**	●	●	●		P		Qualitative	15	
Autoimmune	RF IgM	●	●			WB/S/P		8-200 IU/mL	5
	Anti-CCP Plus	●	●	●		WB/S/P	●	3.5-300 U/mL (Semi-quantitative)	12
	Total IgE	●	●			WB/S/P		1-1,000 IU/mL	12
Other test items	Ferritin	●	●		●	S/P		10-1,000 ng/mL	10
	Vitamin D Neo	●	●			WB/S/P	●	5-100 ng/mL	12
	Calprotectin	●	●			Feces		10-1,000 mg/kg	10
	H. pylori SA	●	●			Feces		Qualitative	12
	KL-6	●	●			S/P		51-3,000 U/mL	10
	mAMP/COC/THC New	●	●			Urine		Qualitative	10
	AMP/EDDP/OPI New	●	●			Urine		Qualitative	10
	BAR/BZO/TCA New	●	●			Urine		Qualitative	10
FEN/KET/MDMA* New	●	●			Urine		Qualitative	10	

* No CE mark

** IGRA-TB Tube required

(★) Available on ichroma™-50 PLUS device

WB = Whole blood, S = Serum, P = Plasma, NS = Nasopharyngeal swab

Compact All-in-one Fluorescence Immuno-analyzer

AFIAS-1

- ▶ Simple procedure with All-in-One cartridges
- ▶ Easy to use without pipetting with proprietary C-tip
- ▶ Quick test results with reliability
- ▶ Small, compact, & light



Specifications

QC/Calibration

- 2 calibrators & 2 controls
- Internal & external controls

Interface

- 5" touch screen
- Built-in thermal printer
- USB port / USB OTG port / Ethernet SD card slot
- LIS/HIS compatible

Memory

- 5,000 patient results
- 5,000 QC results
- 500 ID chips
- 100 User IDs

Analyzer

- 180.6 x 320.6 x 206.4 mm
- 4.0 kg
- 100 – 240 V AC, 50-60 Hz
- Internal temperature control

Multi testing Fluorescence Immuno-analyzer

AFIAS-3

- ▶ AFIAS system runs 3 tests simultaneously
- ▶ Extra tip station – faster TAT
- ▶ Compact system for multiple testing
- ▶ User friendly UI



Specifications

QC/Calibration

- Internal & external controls

Interface

- 7" touch screen
- Built-in thermal printer
- USB port / Ethernet SD card slot / RS232
- LIS/HIS compatible

Memory

- 5,000 patients results
- 5,000 QC results
- 500 ID chips
- 100 User IDs


Analyzer

- 276 x 365 x 313 mm
- 9.3 kg
- 100-240 V AC, 50-60 Hz
- Internal temperature control

Versatile Desktop Fluorescence Immuno-analyzer

AFIAS-6

- ▶ Fast Sample-to-Answer system
- ▶ Easy to use without pipetting with proprietary C-tip
- ▶ Up to 6 different tests simultaneously
- ▶ Reliable test results

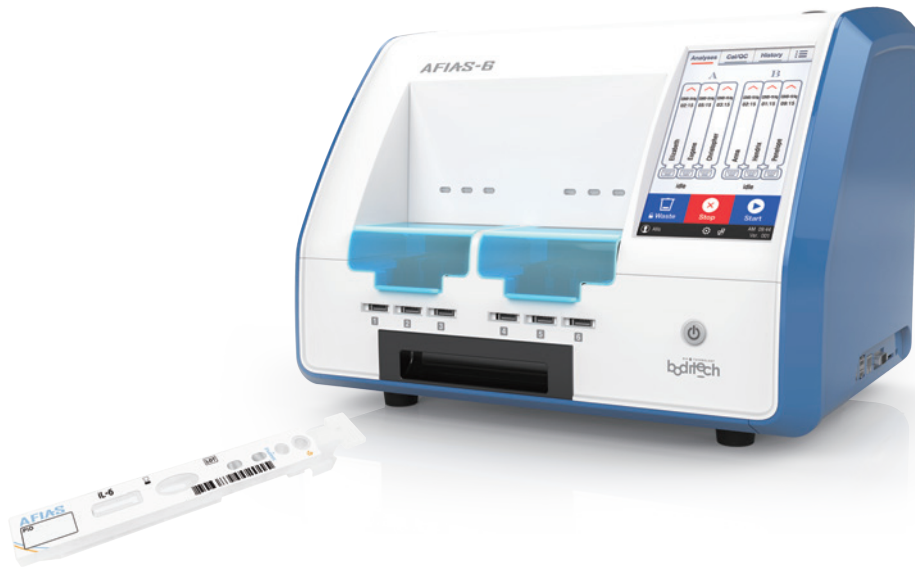

Specifications

QC/Calibration

- 2 calibrators & 2 controls
- Internal & external controls

Interface

- 7" touch screen
- Built-in thermal printer
- USB port / Ethernet
SD card slot / RS232
- LIS/HIS compatible

Memory

- 5,000 patient results
- 5,000 QC results
- 500 ID chips
- 100 User IDs

Analyzer

- 420 x 336 x 293 mm
- 15.1 kg
- 100 – 240 V AC, 50-60 Hz
- Internal temperature control

High-throughput Fluorescence Immunoassay with blood tube

AFIAS-10

- ▶ Sample-to-Answer from blood tube
- ▶ Run up to 10 different tests at once
- ▶ Emergency test first during operation
- ▶ Bidirectional LIS/HIS



Specifications

QC/Calibration

- Internal & external controls

Interface

- 10.1" touch screen
- Built-in thermal printer
- USB port / Ethernet
SD card slot / RS232
- LIS/HIS compatible

Memory

- 10,000 patients & QC results
- 100 ID chips
- 100 User IDs

Analyzer

- 426 x 443 x 395 mm
- 20 kg
- 100-240 V AC, 50-60 Hz
- Internal temperature control

AFIAS Parameters

Category	Item	AFIAS-1	AFIAS-6	AFIAS-3 AFIAS-10	Sample type	C-tip	Working range	Test time (min)
Cardiac	hsCRP	●	●	●	WB/S/P	●	0.1-10 mg/L	3
	D-Dimer	●	●	●	WB/P	●	50-10,000 ng/mL	12
	D-Dimer Neo	●	●	●	WB/P		50-10,000 ng/mL	12
	Tn-I Plus	●	●	●	WB/S/P		0.01-15 ng/mL	12
	CK-MB	●	●	●	WB/S/P		3-100 ng/mL	12
	CK-MB Neo	●	●	●	WB/S/P		3-100 ng/mL	12
	Myoglobin	●	●	●	WB/S/P		2-500 ng/mL	12
	Myoglobin Neo	●	●	●	WB/S/P		2-500 ng/mL	12
	Cardiac Triple	●	●	●	WB/S/P		Tn-I: 0.01-15 ng/mL CK-MB: 3-100 ng/mL Myoglobin: 5-500 ng/mL	12
	Troponin T	●	●	●	WB/S/P	●	10-20,000 pg/mL	12
	BNP	●	●	●	WB/P	●	5-5,000 pg/mL	12
	NT-proBNP	●	●	●	WB/S/P		10-30,000 pg/mL	12
	ST2	●	●	●	WB/S/P		3.1-200 ng/mL	12
	Cancer	PSA	●	●		WB/S/P		0.5-100 ng/mL
PSA Neo		●	●	●	WB/S/P	●	0.1-100 ng/mL	15
Free PSA		●	●	●	WB/S/P	●	0.05-50 ng/mL	12
AFP		●	●	●	WB/S/P		5-350 ng/mL	15
CEA		●	●	●	WB/S/P		1-500 ng/mL	15
Cyfra21-1		●	●	●	S/P		1-500 ng/mL	12
CA19-9		●	●	●	S/P		8-1,000 U/mL	12
CA125		●	●	●	S/P		5-700 U/mL	12
Diabetes	HbA1c	●	●	●	WB	●	(NGSP) 4-15%	10
	HbA1c Neo	●	●	●	WB	●	(NGSP) 4-15%	10
	Microalbumin	●	●	●	Urine		2-300 mg/L	12
	Insulin	●	●	●	WB/S/P	●	2-300 µIU/mL	12
Hormone	TSH	●	●	●	WB/S/P	●	0.09-100 µIU/mL	12
	TSH Plus	●	●	●	WB/S/P	●	0.08-50 µIU/mL	12
	T3	●	●	●	S/P		0.77-7.7 nmol/L	10
	T4	●	●	●	S/P		10.23-300 nmol/L	10
	Free T4	●	●	●	WB/S/P	●	1-100 pmol/L	12
	FSH	●	●	●	WB/S/P		1-100 mIU/mL	12
	Total βhCG	●	●	●	WB/S/P		5-50,000 mIU/mL	15
	β-HCG Plus	●	●	●	WB/S/P	●	2-1,500 mIU/mL	12
	LH	●	●	●	WB/S/P		1-100 mIU/mL	12
	PRL	●	●	●	WB/S/P		1-100 ng/mL	10
	Progesterone	●	●	●	S/P		4.45-127.2 nmol/L	15
	Testosterone	●	●	●	S/P		0.5-12 ng/mL	15
	Cortisol	●	●	●	WB/S/P		80-800 nmol/L	10
	AMH	●	●	●	S/P		0.02-15 ng/mL	12
Estradiol* New	●	●	●	WB/S/P		20-3,000 pg/mL	20	
PTH	●	●	●	WB/S/P		30-3,000 pg/mL	17	

* No CE mark

WB = Whole blood, S = Serum, P = Plasma, NS = Nasopharyngeal swab

AFIAS Parameters

Category	Item	AFIAS-1	AFIAS-6	AFIAS-3 AFIAS-10	Sample type	C-tip	Working range	Test time (min)	
Infection	CRP	●	●	●	WB/S/P	●	0.5-200 mg/L	3	
	MxA/CRP	●	●	●	WB	●	MxA: 10-300 ng/mL CRP: 1-200 mg/L	12	
	PCT	●	●	●	WB/S/P		0.1-100 ng/mL	12	
	PCT X	●	●	●	WB/S/P		0.1-100 ng/mL	12	
	PCT Plus	●	●	●	WB/S/P	●	0.02-50 ng/mL	12	
	PCT Plus G	●	●	●	WB/S/P	●	0.02-50 ng/mL	12	
	IL-6	●	●	●	WB/S/P	●	2-2,500 pg/mL	12	
	Carba 5* (OXA-48, KPC-2, NDM-1, IMP-1, VIM-1) New		●	●	●	C		Qualitative	15
	Flu A+B	●	●	●	NS		Qualitative	10	
	RSV	●	●	●	NS		Qualitative	10	
	COVID-19 Ab	●	●	●	WB/S/P	●	Qualitative	10	
	COVID-19 Ag	●	●	●	NS		Qualitative	12	
	COVID-19/Flu Ag Combo	●	●	●	NS		Qualitative	20	
	COVID-19/Flu A+B/ RSV Ag Combo	●	●	●	NS		Qualitative	20	
	Strep A	●	●	●	Throat swab		Qualitative	10	
	HBsAg*	●	●	●	WB/S/P		Qualitative	12	
	Anti-HBs*	●	●	●	WB/S/P		Qualitative	15	
	Anti-HCV*	●	●	●	WB/S/P		Qualitative	12	
	Dengue NS1 Ag	●	●	●	WB/S/P	●	Qualitative	12	
	Dengue IgG/IgM	●	●	●	WB/S/P	●	Qualitative	12	
	NORO	●	●	●	Feces		Qualitative	12	
	ROTA	●	●	●	Feces		Qualitative	12	
	Rota/Adeno	●	●	●	Feces		Qualitative	12	
IGRA-TB**	●	●	●	P		Qualitative	15		
HIV 1/2 Ab*	●	●	●	WB/S/P	●	Qualitative	10		
Autoimmune	Anti-CCP Plus	●	●	●	WB/S/P	●	3.2-300 U/mL	12	
	Total IgE	●	●	●	WB/S/P		1-1,000 IU/mL	12	
TDM (Therapeutic Drug Monitoring)	Infliximab	●	●	●	WB/S/P	●	0.2-50 µg/mL	10	
	Adalimumab	●	●	●	WB/S/P	●	0.2-50 µg/mL	10	
	Golimumab	●	●	●	WB/S/P	●	0.2-30 µg/mL	10	
	Vedolizumab	●	●	●	WB/S/P	●	2-60 µg/mL	10	
	Ustekinumab	●	●	●	WB/S/P	●	0.5-20 µg/mL	10	
	Etanercept	●	●	●	WB/S/P	●	0.2-10 µg/mL	10	
	Trastuzumab	●	●	●	WB/S/P	●	3-150 µg/mL	10	
	Total Anti-Infliximab	●	●	●	S/P		8-250 AU/mL	22	
	Free Anti-Infliximab	●	●	●	WB/S	●	4-250 AU/mL	12	
	Free Anti-Adalimumab	●	●	●	WB/S	●	3-200 AU/mL	12	
	Free Anti-Golimumab	●	●	●	WB/S	●	2-40 ng/mL	10	
	Free Anti-Vedolizumab	●	●	●	WB/S	●	10-250 ng/mL	10	
	Free Anti-Ustekinumab	●	●	●	WB/S	●	2.5-100 ng/mL	12	
	Free Anti-Etanercept	●	●	●	WB/S	●	10-100 ng/mL	10	
	Free Anti-Trastuzumab	●	●	●	WB/S	●	8-500 AU/mL	10	
Other test items	sphingotest® penKid® New	●	●	●	WB/P		70-2,500 pmol/L	15	
	Ferritin	●	●	●	S/P		10-1,000 ng/mL	10	
	Vitamin D Neo	●	●	●	WB/S/P	●	5-100 ng/mL	12	
	KL-6	●	●	●	S/P		51-3,000 U/mL	10	
	H. pylori SA	●	●	●	Feces		Qualitative	12	
	Calprotectin	●	●	●	Feces		10-1,000 mg/kg	10	

* No CE mark

** IGRA-TB Tube required

WB = Whole blood, S = Serum, P = Plasma, NS = Nasopharyngeal swab
C = Colony tested from isolated bacterial colonies on culture plates


Total Hemoglobin Meter

hemochroma PLUS

- ▶ Microcuvette with dual sample inlets
- ▶ Capillary blood or tube blood

Specifications

Principle	Absorptiometry
Sample Types	Whole blood
Sample volume	15 µL
Detection range	0-27.0 g/dL
Reading time	3 seconds
Memory	1,000 tests
Analyzer	106.5 x 151.0 x 38.5 mm
Power	Batteries (AA×4) or USB charger Serial printer connection

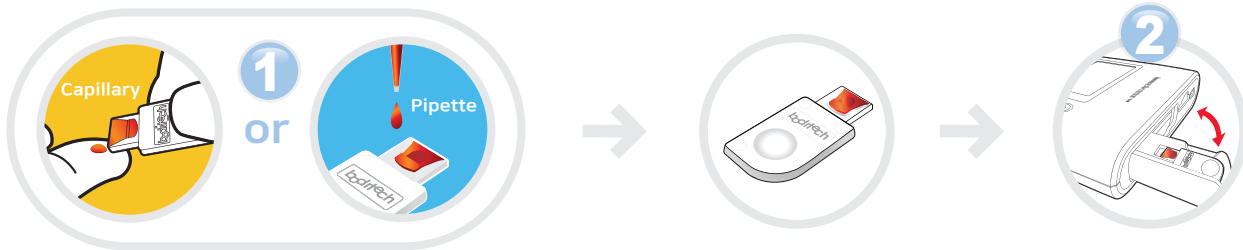

Boditech Quick™

Rapid Diagnostic Test

- ▶ On-site diagnostics with naked eyes
- ▶ Simple test procedure
- ▶ Fast and reliable result



Category	Item	Testing type	Sample type	Test time (min)
Infection	Boditech Quick™ HIV 1/2 Ab*	IVD use	WB/S/P	15
	Boditech Quick™ Syphilis	IVD use	WB/S/P	15
	Boditech Quick™ HbsAg*	IVD use	WB/S/P	15
	Boditech Quick™ Anti-HCV*	IVD use	WB/S/P	20
	Boditech Quick™ Dengue NS1	IVD use	WB/S/P	15
	Boditech Quick™ Dengue IgM/IgG	IVD use	WB/S/P	15
	Boditech Quick™ COVID-19 Ag Nasal	IVD use	Nasopharyngeal swab Nasal swab	15
	Boditech Quick™ COVID-19 Ag Saliva	IVD use Self testing*	Saliva	15

* No CE mark

Fully Automated Chemistry Analyzer

Alchemis

- ▶ Portable & Accessible device
- ▶ Simple 3-step workflow
- ▶ Nanofilter for WB compatibility
- ▶ Multiplex testing
- ▶ Optimized & Expandable panels



	AST	ALT	ALB	GGT	ALP	CREA	BUN	BUN/CREA*	eGFR*	GLU	TC	TG	HDL-C	LDL-C*	TC/HDL
LiverKidney Kit	●	●	●	●	●	●	●	●	●						
Lipid Kit										●	●	●	●	●	●
LiverLipid Kit	●	●	●	●							●	●	●	●	●

Specifications

QC/Calibration

- External controls

Interface

- 5" touch screen
- Built-in thermal printer
- USB port/ Ethernet

Memory

- 10,000 patients

Analyzer

- 144 x 226 x 162 mm
- 1.5 kg
- 100-240 V AC, 50-60 Hz



*Calculated

Advanced Compact Immunofluorescence Analyzer

Vet chroma

- ▶ High performance with proven reliability
- ▶ Small, lightweight, and space-saving design
- ▶ Multi-test functionality
- ▶ Intuitive, and user-friendly interface
- ▶ Simplify your process with ease using all-in-one tube*



Parameters	 Canine	 Feline
Category	Canine	Feline
Hormone	Cortisol / T4 Progesterone / TSH	Cortisol / T4
Inflammation	cCRP / cPL	fSAA / fPL
Infection	Canine 3D / Helicobacter SA / Giardia	Helicobacter SA / Giardia
Cardiac	cNT-proBNP / Tn-I	fNT-proBNP
Others	AFP / D-Dimer / SDMA	SDMA

* Refer to the package insert for additional information



Your life, Our inspiration

Boditech Med Inc.



Boditech Med Inc.

43, Geodudanji 1-gil, Dongnae-myeon,
Chuncheon-si, Gang-won-do 24398, Republic of Korea
Tel: +82-33-243-1400, Fax: +82-33-243-9373
sales@boditech.co.kr/www.boditech.co.kr

Distributed by